




# QC™ Mobile Dispensing System Wall Chart





BATHROOM

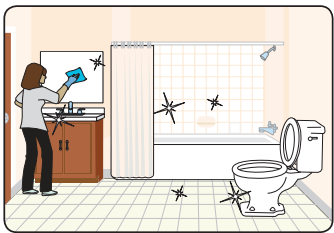

PRODUCT DISPENSER LABEL



- 1. Wear appropriate PPE and place floor signs where needed.
- 2. Apply product with a spray bottle when using bottle head OR foam directly when using a foaming head.
- 3. Allow product to soak. *If using a disinfectant, allow for appropriate contact time.\**
- 4. Wipe clean and dry with clean cloth, sponge or mop. Rinse as needed.

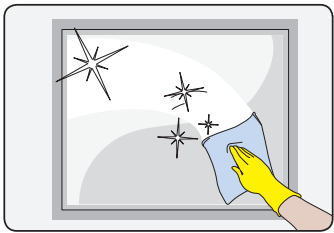


GLASS



PRODUCT DISPENSER LABEL



- 1. Wear appropriate PPE and place floor signs where needed.
- 2. Spray microfiber or cloth with product and wipe product onto surface.
- 3. Wipe clean and dry with clean cloth, towel, sponge or squeegee.
- 4. If needed, polish with clean cloth.

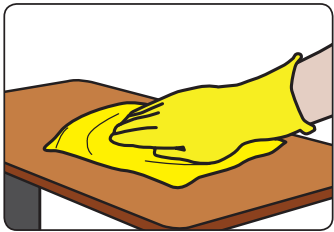



SURFACE



PRODUCT DISPENSER LABEL



- 1. Wear appropriate PPE and place floor signs where needed.
- 2a. Spray product onto microfiber OR fill mop bucket with product and soak microfiber cloths.
- 2b. Apply product directly to surface with sponge or mop.
- 3. Allow a few minutes to work. *If using a disinfectant, allow for appropriate contact time.\** Rinse as needed.

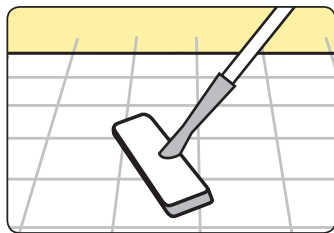





FLOOR




PRODUCT DISPENSER LABEL



- 1. Wear appropriate PPE and place floor signs where needed.
- 2a. If using a foamer, spray product onto surface. Scrub and rinse.
- 2b. If using a mop bucket, mop in a figure 8 pattern with overlaps.
- 2c. If using a scrubber, use red pad for cleaning.




Spray Bottle/  
Mop Bucket Head

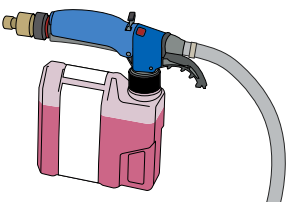


Foam/Rinse Head


## PRODUCT REPLACEMENT STEPS

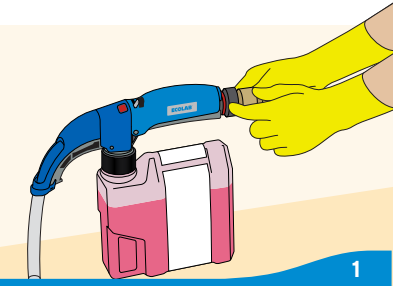


1  
Detach dispensing head from hose.

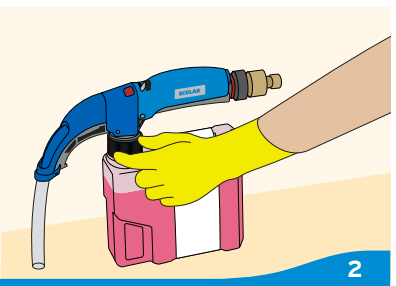

2  
Unscrew empty cartridge from MDS unit.

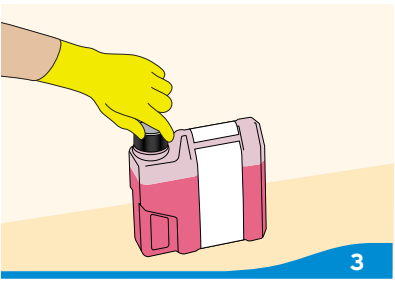

3  
Remove outer cap from new cartridge.

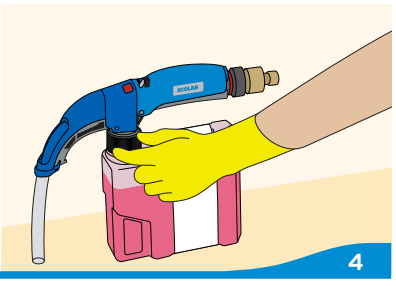

4  
Screw on new cartridge from MDS unit.

Everywhere It Matters.™

\* When using disinfectants, refer to the product label for specific use instructions, rinse requirements and required contact time.

1 800 35 CLEAN